

ROOM NO.
1A02
1A06
1A24
1A28
1A32

# NULOOK REFRESH

(M/N: FW1207-NU-GEN-P)

FOR PRESENTATION  
PURPOSES ONLY  
Nov-23-2021  
NOT FOR  
CONSTRUCTION USE

## DRAWING # 01

TYPE:	LDR - TYPE 1 LDR - TYPE 2	QUANTITY:	5
-------	------------------------------	-----------	---


## AS SHOWN

### SYSTEM DETAILS

SYM	QTY	DESCRIPTION
NU	1	NULOOK REFRESH: 147 1/2" x 85" x 4 3/4"
O	2	AMICO GAS OUTLET, OXYGEN
V	2	AMICO GAS OUTLET, VACUUM
N2	2	RECEPTACLE - DUPLEX IVORY
USB	2	USB RECEPTACLE - DUPLEX IVORY
E4	1	RECEPTACLE - QUAD RED
SN1	4	SWITCH - S.P.S.T. IVORY
SO	2	PROVISION - SCONCE 1G
TL	2	PROVISION - TELEPHONE 1G
NC	1	PROVISION - NURSE CALL 3G
BB	1	VERTICAL BED BUMPER - PAIR
RP	1	RESIN PANEL - 47 1/2" x 24" (W x H)
	1	LED PANEL - 47 1/2" x 24" (W x H)
SLM	2	VACUUM SLIDE
SD	1	SLIDING DOOR - 22" x 18"


#### NOTE:

- HANGING BRACKET SUPPLIED BY AMICO.
- BLOCKING TO BE SUPPLIED BY OTHERS. LOCATION TO BE DETERMINED DURING SUBMITTAL PHASE.
- CUSTOMER ACKNOWLEDGES THAT ON-SITE CONDITIONS MAY DIFFER FROM ROOM TO ROOM. AMICO WILL NOT BE HELD LIABLE IF HEADWALL MEASUREMENT DISCREPANCIES OCCUR ON-SITE.
- RESIN PANEL TO BE 3-FORM GROUP C, 3/8" GAUGE, FAIRY TALE VAPOR W05 WITH SANDSTONE FINISH.
- RESIN PANEL ARE TO BE BACKLIT WITH AMICO LED PANEL.
- RESIN PANEL, LED STRIPS AND LED TERMINATION BOX TO BE SHIPPED LOOSE AND INSTALLED ON SITE BY OTHERS - REFER TO INSTALLATION INSTRUCTIONS PRIOR TO ASSEMBLY.
- HORIZONTAL OVERHANGING IS NOT SHOWN ON THE DRAWING. CUSTOMER TO CONFIRM REQUIRED HEIGHT BETWEEN THE CEILING AND TOP OF HEADWALL, MAX. 6" OVERHANG IS PROVIDED.
- SCONCES TO BE PROVIDED AND INSTALLED BY OTHERS, BLOCKING AND PROVISION PROVIDED BY AMICO.

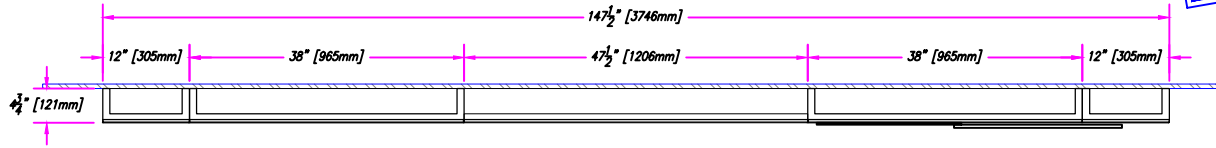

DOOR SIDE

WINDOW SIDE

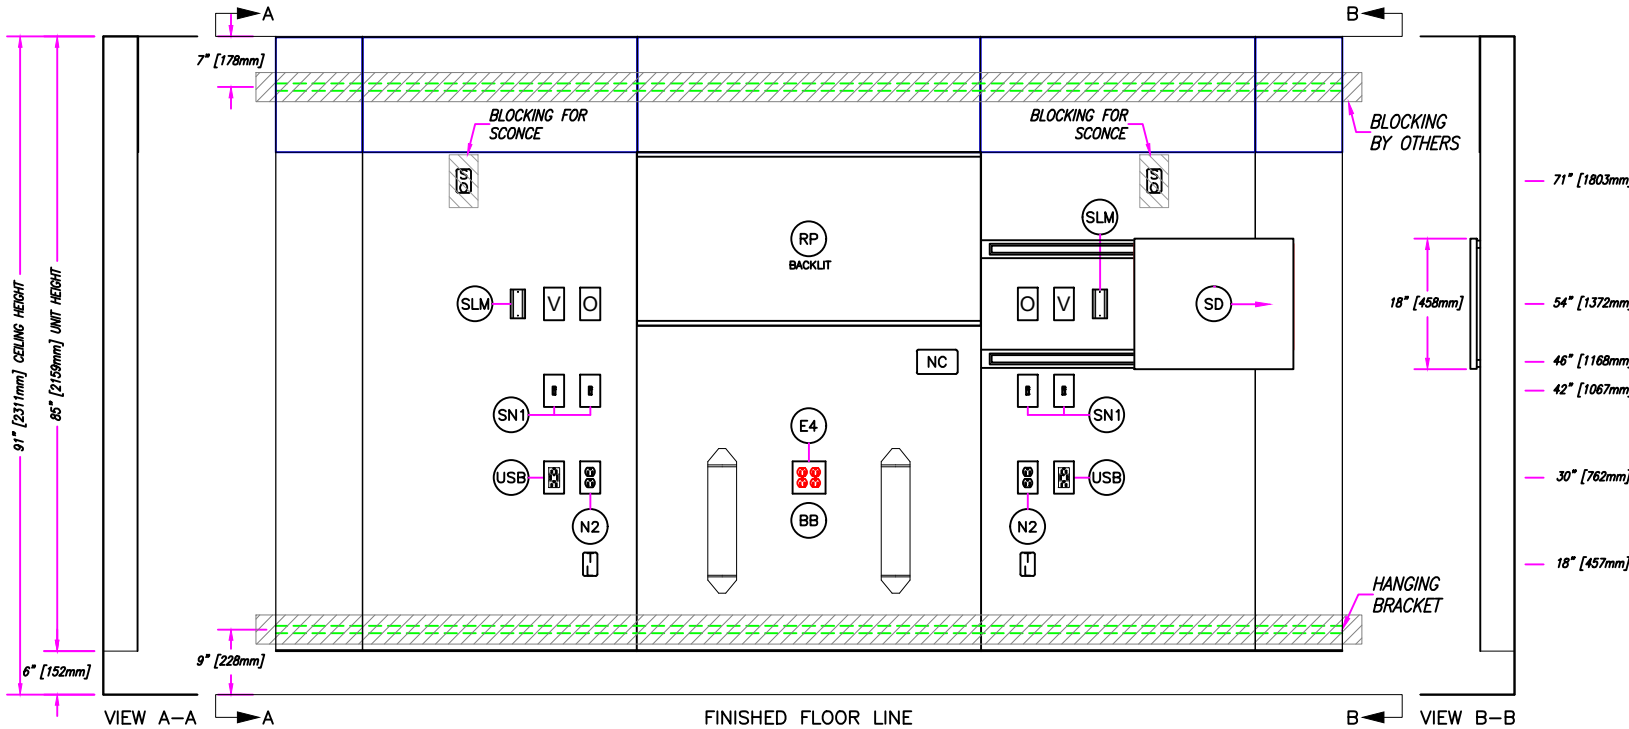

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE

DATE

PHONE NO.

HOSPITAL	RICHMOND UNIVERSITY MEDICAL CENTER	NURSE CALL	MFGR. : TBC	MODEL No. : TBC
LOCATION	STATEN ISLAND, NY	GAS OUTLETS	MFGR. : AMICO	TYPE CONNECTION : TBC
	UNIT AS SHOWN - N.T.S.	FINISH	TBC	CEILING HEIGHT 7' - 7"



85 Fulton Way  
Richmond Hill, Ontario  
L4B 2N4, CANADA  
Toll-Free: 1-877-482-6428(T)  
1-866-440-4986(F)  
Tel: (905) 764-0800  
Fax: (905) 764-0862

QUOTE No. AC014104
REV. BY: SLIU PROJECT PM: N/A
DATE: Nov-23-2021
REV. NO: 03

ROOM NO.
1A04
1A08
1A22
1A26
1A30

# NULOOK REFRESH

(M/N: FW1207-NU-GEN-P)

FOR PRESENTATION  
PURPOSES ONLY  
Nov-23-2021  
NOT FOR  
CONSTRUCTION USE

## DRAWING # 01.1

TYPE:	LDR - TYPE 1 LDR - TYPE 2	QUANTITY:	5
-------	------------------------------	-----------	---


## MIRRORED

### SYSTEM DETAILS

SYM	QTY	DESCRIPTION
NU	1	NULOOK REFRESH: 147 1/2" x 85" x 4 3/4"
O	2	AMICO GAS OUTLET, OXYGEN
V	2	AMICO GAS OUTLET, VACUUM
N2	2	RECEPTACLE - DUPLEX IVORY
USB	2	USB RECEPTACLE - DUPLEX IVORY
E4	1	RECEPTACLE - QUAD RED
SN1	4	SWITCH - S.P.S.T. IVORY
SO	2	PROVISION - SCONCE 1G
TL	2	PROVISION - TELEPHONE 1G
NC	1	PROVISION - NURSE CALL 3G
BB	1	VERTICAL BED BUMPER - PAIR
RP	1	RESIN PANEL - 47 1/2" x 24" (W x H)
	1	LED PANEL - 47 1/2" x 24" (W x H)
SLM	2	VACUUM SLIDE
SD	1	SLIDING DOOR - 22" x 18"


**NOTE:**

- HANGING BRACKET SUPPLIED BY AMICO.
- BLOCKING TO BE SUPPLIED BY OTHERS. LOCATION TO BE DETERMINED DURING SUBMITTAL PHASE.
- CUSTOMER ACKNOWLEDGES THAT ON-SITE CONDITIONS MAY DIFFER FROM ROOM TO ROOM. AMICO WILL NOT BE HELD LIABLE IF HEADWALL MEASUREMENT DISCREPANCIES OCCUR ON-SITE.
- RESIN PANEL TO BE 3-FORM GROUP C, 3/8" GAUGE, FAIRY TALE VAPOR W05 WITH SANDSTONE FINISH.
- RESIN PANEL ARE TO BE BACKLIT WITH AMICO LED PANEL.
- RESIN PANEL, LED STRIPS AND LED TERMINATION BOX TO BE SHIPPED LOOSE AND INSTALLED ON SITE BY OTHERS - REFER TO INSTALLATION INSTRUCTIONS PRIOR TO ASSEMBLY.
- HORIZONTAL OVERHANGING IS NOT SHOWN ON THE DRAWING. CUSTOMER TO CONFIRM REQUIRED HEIGHT BETWEEN THE CEILING AND TOP OF HEADWALL, MAX. 6" OVERHANG IS PROVIDED.
- SCONCES TO BE PROVIDED AND INSTALLED BY OTHERS, BLOCKING AND PROVISION PROVIDED BY AMICO.

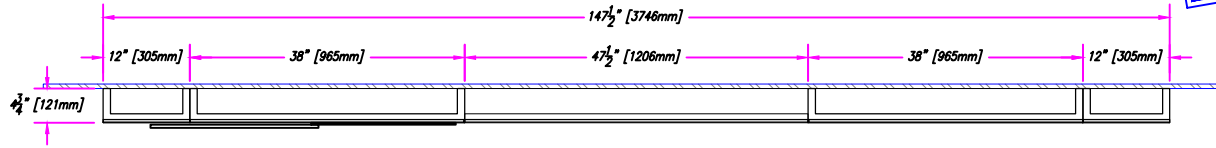

WINDOW SIDE

DOOR SIDE

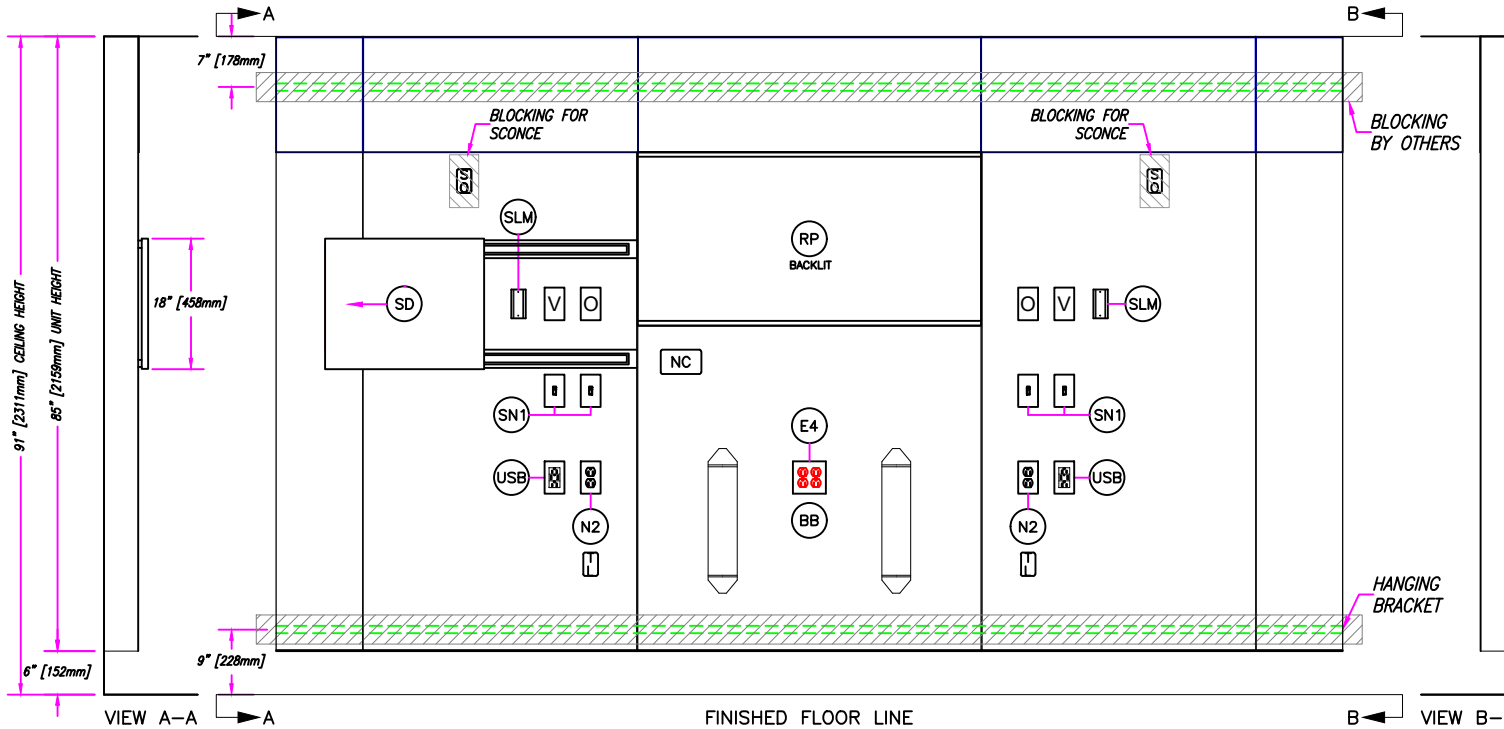

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE

DATE

PHONE NO.

HOSPITAL	RICHMOND UNIVERSITY MEDICAL CENTER	NURSE CALL	MFGR. : TBC	MODEL No. : TBC
LOCATION	STATEN ISLAND, NY	GAS OUTLETS	MFGR. : AMICO	TYPE CONNECTION : TBC
	UNIT AS SHOWN - N.T.S.	FINISH	TBC	CEILING HEIGHT 7' - 7"

85 Fulton Way  
Richmond Hill, Ontario  
L4B 2N4, CANADA  
Toll-Free: 1-877-482-6428(T)  
1-866-440-4986(F)  
Tel: (905) 764-0800  
Fax: (905) 764-0862

QUOTE No. AC014104  
REV. BY: SLIU  
PROJECT PM: N/A  
DATE: Nov-23-2021  
REV. NO: 03

www.amico.com

ROOM NO.
2A02
2A06
2A10
2A14

# NULOOK REFRESH

(M/N: FW1207-NU-GEN-P)

FOR PRESENTATION  
PURPOSES ONLY  
Nov-23-2021  
NOT FOR  
CONSTRUCTION USE

## DRAWING # 02

TYPE:	QUANTITY:
LDR - TYPE 3	4


### AS SHOWN

#### SYSTEM DETAILS

SYM	QTY	DESCRIPTION
NU	1	NULOOK REFRESH: 147 1/2" x 85" x 4 3/4"
O	2	AMICO GAS OUTLET, OXYGEN
V	2	AMICO GAS OUTLET, VACUUM
N2	2	RECEPTACLE - DUPLEX IVORY
USB	2	USB RECEPTACLE - DUPLEX IVORY
SN1	4	SWITCH - S.P.S.T. IVORY
SO	2	PROVISION - SCONCE 1G
TL	2	PROVISION - TELEPHONE 1G
NC	1	PROVISION - NURSE CALL 3G
BB	1	VERTICAL BED BUMPER - PAIR
RP	1	RESIN PANEL - 47 1/2" x 24" (W x H)
	1	LED PANEL - 47 1/2" x 24" (W x H)
SLM	2	VACUUM SLIDE
SD	1	SLIDING DOOR - 22" x 18"


#### NOTE:

- HANGING BRACKET SUPPLIED BY AMICO.
- BLOCKING TO BE SUPPLIED BY OTHERS. LOCATION TO BE DETERMINED DURING SUBMITTAL PHASE.
- CUSTOMER ACKNOWLEDGES THAT ON-SITE CONDITIONS MAY DIFFER FROM ROOM TO ROOM. AMICO REQUIRES MEASUREMENTS FOR ALL ROOMS. AMICO WILL NOT BE HELD LIABLE IF HEADWALL MEASUREMENT DISCREPANCIES OCCUR ON-SITE.
- RESIN PANEL TO BE 3-FORM GROUP C, 3/8" GAUGE, FAIRY TALE VAPOR W05 WITH SANDSTONE FINISH.
- RESIN PANEL ARE TO BE BACKLIT WITH AMICO LED PANEL.
- RESIN PANEL, LED STRIPS AND LED TERMINATION BOX TO BE SHIPPED LOOSE AND INSTALLED ON SITE BY OTHERS - REFER TO INSTALLATION INSTRUCTIONS PRIOR TO ASSEMBLY.
- HORIZONTAL OVERHANGING IS NOT SHOWN ON THE DRAWING. CUSTOMER TO CONFIRM REQUIRED HEIGHT BETWEEN THE CEILING AND TOP OF HEADWALL, MAX. 6" OVERHANG IS PROVIDED.
- SCONCES TO BE PROVIDED AND INSTALLED BY OTHERS, BLOCKING AND PROVISION PROVIDED BY AMICO.

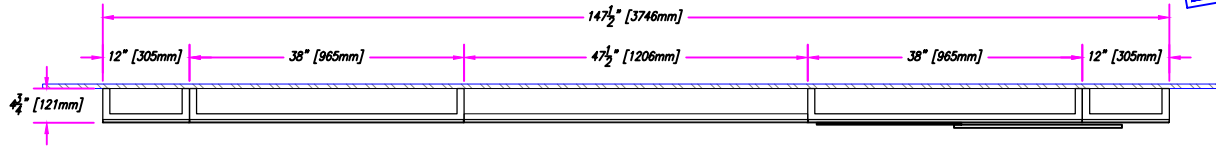

DOOR SIDE

WINDOW SIDE

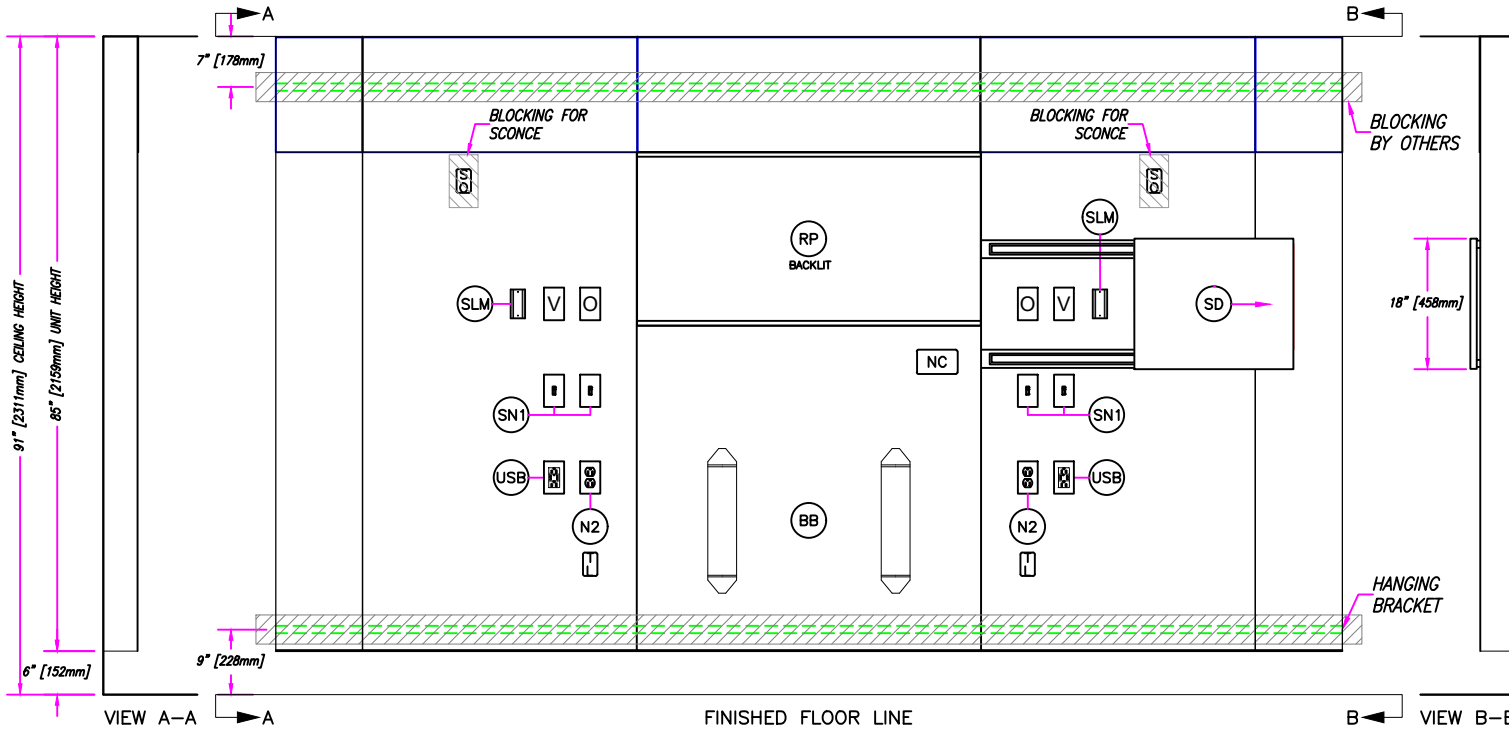

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE

DATE

PHONE NO.

HOSPITAL	RICHMOND UNIVERSITY MEDICAL CENTER	NURSE CALL	MFGR. : TBC	MODEL No. : TBC
LOCATION	STATEN ISLAND, NY	GAS OUTLETS	MFGR. : AMICO	TYPE CONNECTION : TBC
	UNIT AS SHOWN - N.T.S.	FINISH	TBC	CEILING HEIGHT 7' - 7"



85 Fulton Way  
Richmond Hill, Ontario  
L4B 2N4, CANADA  
Toll-Free: 1-877-482-6428(T)  
1-866-440-4986(F)  
Tel: (905) 764-0800  
Fax: (905) 764-0862

QUOTE No.  
AC014104  
REV. BY: SLIU  
PROJECT PM: N/A  
DATE: Nov-23-2021  
REV. NO: **03**

www.amico.com

ROOM NO.
2A04
2A08
2A12

# NULOOK REFRESH

(M/N: FW1207-NU-GEN-P)

FOR PRESENTATION  
PURPOSES ONLY  
Nov-23-2021  
NOT FOR  
CONSTRUCTION USE

## DRAWING # 02.1

TYPE:	QUANTITY:
LDR - TYPE 3	3


### MIRRORED

#### SYSTEM DETAILS

SYM	QTY	DESCRIPTION
NU	1	NULOOK REFRESH: 147 1/2" x 85" x 4 3/4"
O	2	AMICO GAS OUTLET, OXYGEN
V	2	AMICO GAS OUTLET, VACUUM
N2	2	RECEPTACLE - DUPLEX IVORY
USB	2	USB RECEPTACLE - DUPLEX IVORY
SN1	4	SWITCH - S.P.S.T. IVORY
SO	2	PROVISION - SCONCE 1G
TL	2	PROVISION - TELEPHONE 1G
NC	1	PROVISION - NURSE CALL 3G
BB	1	VERTICAL BED BUMPER - PAIR
RP	1	RESIN PANEL - 47 1/2" x 24" (W x H)
	1	LED PANEL - 47 1/2" x 24" (W x H)
SLM	2	VACUUM SLIDE
SD	1	SLIDING DOOR - 22" x 18"


#### NOTE:

- HANGING BRACKET SUPPLIED BY AMICO.
- BLOCKING TO BE SUPPLIED BY OTHERS. LOCATION TO BE DETERMINED DURING SUBMITTAL PHASE.
- CUSTOMER ACKNOWLEDGES THAT ON-SITE CONDITIONS MAY DIFFER FROM ROOM TO ROOM. AMICO WILL NOT BE HELD LIABLE IF HEADWALL MEASUREMENT DISCREPANCIES OCCUR ON-SITE.
- RESIN PANEL TO BE 3-FORM GROUP C, 3/8" GAUGE, FAIRY TALE VAPOR W05 WITH SANDSTONE FINISH.
- RESIN PANEL ARE TO BE BACKLIT WITH AMICO LED PANEL.
- RESIN PANEL, LED STRIPS AND LED TERMINATION BOX TO BE SHIPPED LOOSE AND INSTALLED ON SITE BY OTHERS - REFER TO INSTALLATION INSTRUCTIONS PRIOR TO ASSEMBLY.
- HORIZONTAL OVERHANGING IS NOT SHOWN ON THE DRAWING. CUSTOMER TO CONFIRM REQUIRED HEIGHT BETWEEN THE CEILING AND TOP OF HEADWALL, MAX. 6" OVERHANG IS PROVIDED.
- SCONCES TO BE PROVIDED AND INSTALLED BY OTHERS, BLOCKING AND PROVISION PROVIDED BY AMICO.

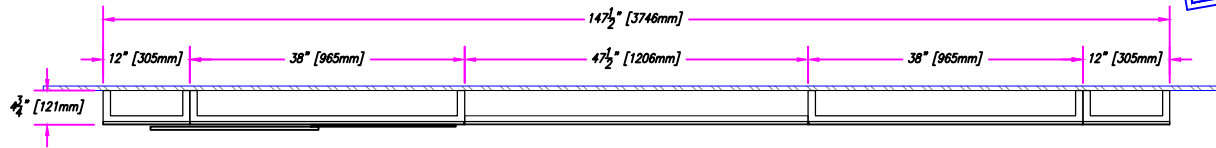

WINDOW SIDE

DOOR SIDE

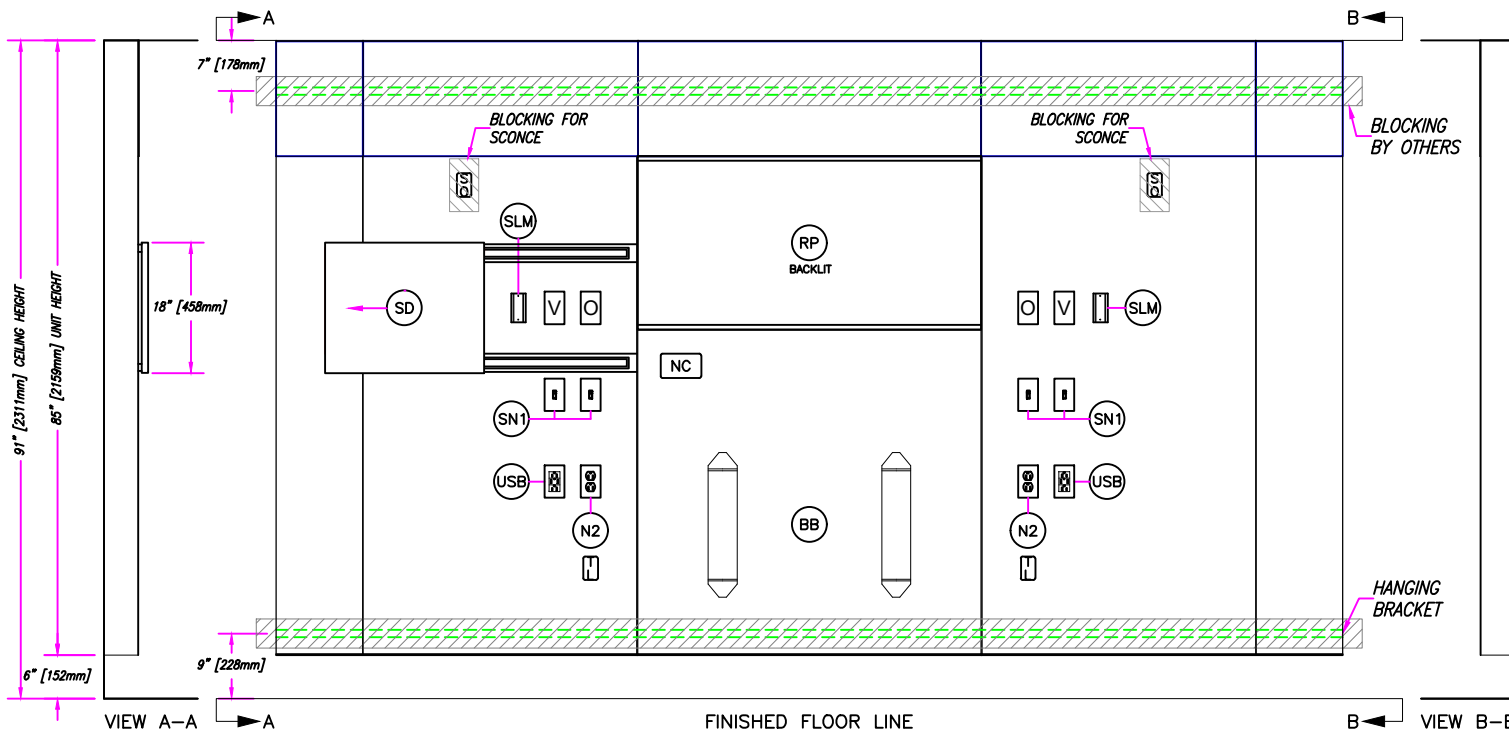

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE

DATE

PHONE NO.

HOSPITAL	RICHMOND UNIVERSITY MEDICAL CENTER	NURSE CALL	MFGR. : TBC	MODEL No. : TBC
LOCATION	STATEN ISLAND, NY	GAS OUTLETS	MFGR. : AMICO	TYPE CONNECTION : TBC
	UNIT AS SHOWN - N.T.S.	FINISH	TBC	CEILING HEIGHT 7' - 7"



85 Fulton Way  
Richmond Hill, Ontario  
L4B 2N4, CANADA  
Toll-Free: 1-877-482-6428(T)  
1-866-440-4986(F)  
Tel: (905) 764-0800  
Fax: (905) 764-0862

QUOTE No.  
AC014104  
REV. BY: SLIU  
PROJECT PM: N/A  
DATE: Nov-23-2021  
REV. NO: **03**

www.amico.com

ROOM NO.
1A36
1A40

# NULOOK REFRESH

(M/N: FW1207-NU-GEN-P)

FOR PRESENTATION  
PURPOSES ONLY  
Nov-23-2021  
NOT FOR  
CONSTRUCTION USE

## DRAWING # 03

TYPE:	QUANTITY:
LDR - TYPE 4	2



### AS SHOWN

#### SYSTEM DETAILS

SYM	QTY	DESCRIPTION
NU	1	NULOOK REFRESH: 66" x 85" x 9"
NU	2	NULOOK REFRESH: 41" x 85" x 3 1/4"
O	4	AMICO GAS OUTLET, OXYGEN
V	6	AMICO GAS OUTLET, VACUUM
E2	2	RECEPTACLE - DUPLEX RED
N2	2	RECEPTACLE - DUPLEX IVORY
USB	2	USB RECEPTACLE - DUPLEX IVORY
SN1	4	SWITCH - S.P.S.T. IVORY
SO	2	PROVISION - SCONCE 1G
NC	1	PROVISION - NURSE CALL 3G
BB	2	VERTICAL BED BUMPER - PAIR
RP	2	RESIN PANEL - 41" x 24" (W x H)
	2	LED PANEL - 47 1/2" x 24" (W x H)
SLM	2	VACUUM SLIDE
DB	2	CUTOUT - DIALYSIS BOX 17"x14"

#### NOTE:

- HANGING BRACKET SUPPLIED BY AMICO.
- BLOCKING TO BE SUPPLIED BY OTHERS. LOCATION TO BE DETERMINED DURING SUBMITTAL PHASE.
- CUSTOMER ACKNOWLEDGES THAT ON-SITE CONDITIONS MAY DIFFER FROM ROOM TO ROOM. AMICO REQUIRES MEASUREMENTS FOR ALL ROOMS. AMICO WILL NOT BE HELD LIABLE IF HEADWALL MEASUREMENT DISCREPANCIES OCCUR ON-SITE.
- RESIN PANEL TO BE 3-FORM GROUP C, 3/8" GAUGE, FAIRY TALE VAPOR WO5 WITH SANDSTONE FINISH.
- RESIN PANEL ARE TO BE BACKLIT WITH AMICO LED PANEL.
- RESIN PANEL, LED STRIPS AND LED TERMINATION BOX TO BE SHIPPED LOOSE AND INSTALLED ON SITE BY OTHERS - REFER TO INSTALLATION INSTRUCTIONS PRIOR TO ASSEMBLY.
- DIALYSIS BOX CUTOUT IS PROVIDED. CLEARANCE AREA AROUND TO BE 17" x 14". CLIENT TO CONFIRM IF MORE CLEARANCE IS REQUIRED.
- DIALYSIS BOX AND INSTALLATION PROVIDED BY OTHERS.
- GFCI RECEPTACLES AVAILABLE BY REQUEST AT AN ADDITION CHARGE.
- HORIZONTAL OVERHANGING IS NOT SHOWN ON THE DRAWING. CUSTOMER TO CONFIRM REQUIRED HEIGHT BETWEEN THE CEILING AND TOP OF HEADWALL. MAX. 6" OVERHANG IS PROVIDED.
- SCONCES TO BE PROVIDED AND INSTALLED BY OTHERS, BLOCKING AND PROVISION PROVIDED BY AMICO.

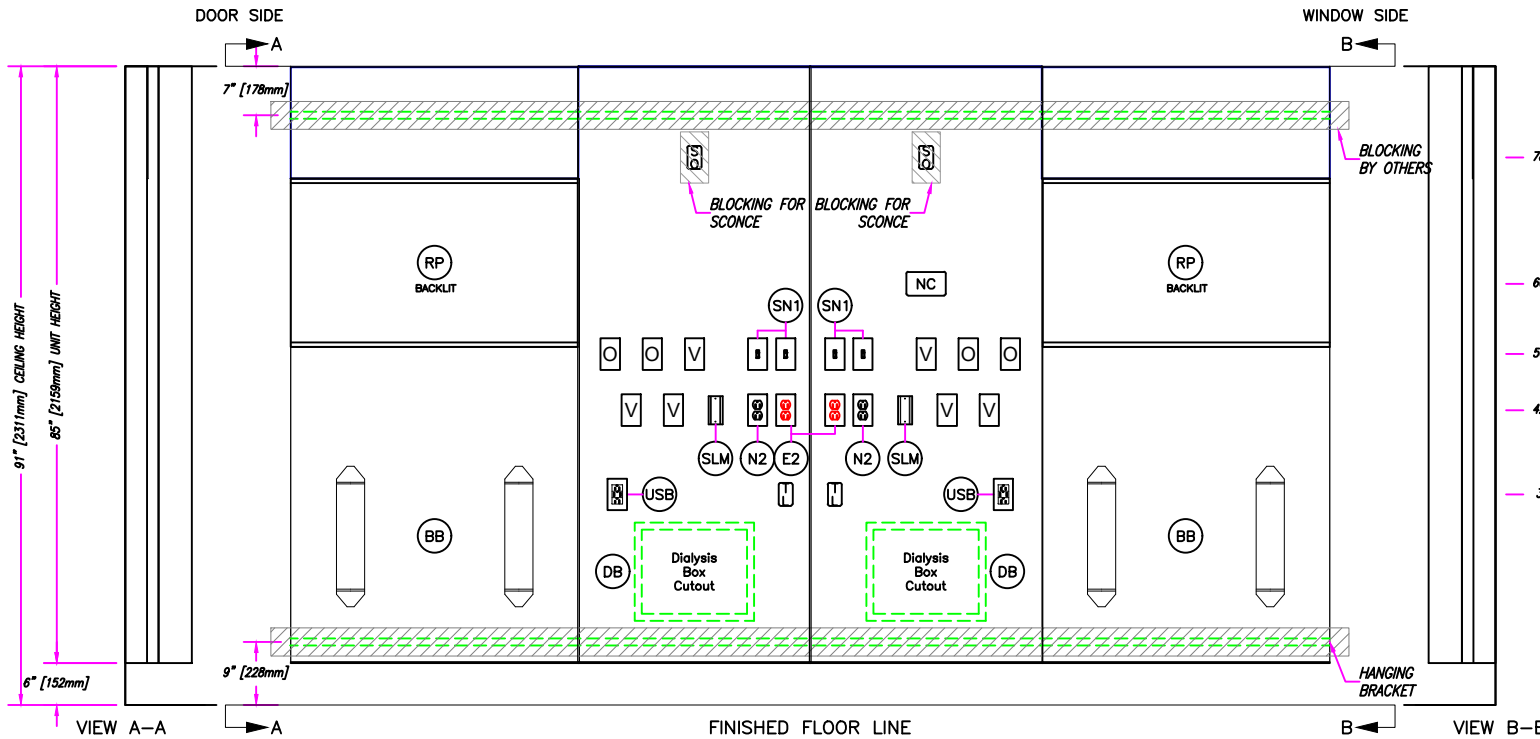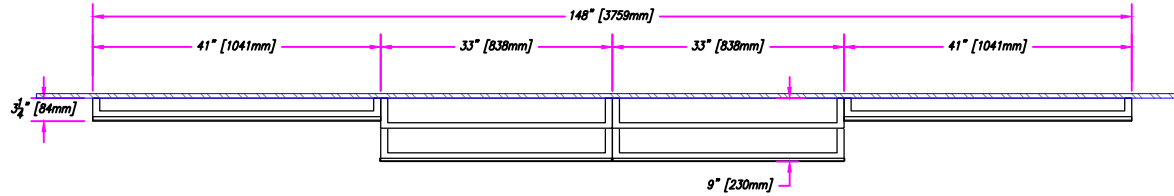

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE

DATE

PHONE NO.

HOSPITAL	RICHMOND UNIVERSITY MEDICAL CENTER	NURSE CALL	MFGR. : TBC	MODEL No. : TBC
LOCATION	STATEN ISLAND, NY	GAS OUTLETS	MFGR. : AMICO	TYPE CONNECTION : TBC
	UNIT AS SHOWN - N.T.S.	FINISH	TBC	CEILING HEIGHT 7' - 7"



85 Fulton Way  
Richmond Hill, Ontario  
L4B 2N4, CANADA  
Toll-Free: 1-877-482-6428(T)  
1-866-440-4986(F)  
Tel: (905) 764-0800  
Fax: (905) 764-0862

QUOTE No.  
AC014104  
REV. BY: SLIU  
PROJECT PM: N/A  
DATE: Nov-23-2021  
REV. NO: 03

ROOM NO.
1A34
1A38

# NULOOK REFRESH

(M/N: FW1207-NU-GEN-P)

FOR PRESENTATION  
PURPOSES ONLY  
Nov-23-2021  
NOT FOR  
CONSTRUCTION USE

## DRAWING # 03.1



TYPE:	QUANTITY:
LDR - TYPE 4	2

### MIRRORED

#### SYSTEM DETAILS

SYM	QTY	DESCRIPTION
NU	1	NULOOK REFRESH: 66" x 85" x 9"
NU	2	NULOOK REFRESH: 41" x 85" x 3 1/4"
O	4	AMICO GAS OUTLET, OXYGEN
V	6	AMICO GAS OUTLET, VACUUM
E2	2	RECEPTACLE - DUPLEX RED
N2	2	RECEPTACLE - DUPLEX IVORY
USB	2	USB RECEPTACLE - DUPLEX IVORY
SN1	4	SWITCH - S.P.S.T. IVORY
SO	2	PROVISION - SCONCE 1G
NC	1	PROVISION - NURSE CALL 3G
BB	2	VERTICAL BED BUMPER - PAIR
RP	2	RESIN PANEL - 41" x 24" (W x H)
	2	LED PANEL - 47 1/2" x 24" (W x H)
SLM	2	VACUUM SLIDE
DB	2	CUTOUT - DIALYSIS BOX 17"x14"

- NOTE:**
- 78" [1981mm] - HANGING BRACKET SUPPLIED BY AMICO.
  - 60" [1524mm] - BLOCKING TO BE SUPPLIED BY OTHERS. LOCATION TO BE DETERMINED DURING SUBMITTAL PHASE.
  - 50" [1270mm] - CUSTOMER ACKNOWLEDGES THAT ON-SITE CONDITIONS MAY DIFFER FROM ROOM TO ROOM. AMICO REQUIRES MEASUREMENTS FOR ALL ROOMS. AMICO WILL NOT BE HELD LIABLE IF HEADWALL MEASUREMENT DISCREPANCIES OCCUR ON-SITE.
  - 42" [1067mm] - RESIN PANEL TO BE 3-FORM GROUP C, 3/8" GAUGE, FAIRY TALE VAPOR WO5 WITH SANDSTONE FINISH.
  - 30" [762mm] - RESIN PANEL ARE TO BE BACKLIT WITH AMICO LED PANEL.
  - RESIN PANEL, LED STRIPS AND LED TERMINATION BOX TO BE SHIPPED LOOSE AND INSTALLED ON SITE BY OTHERS - REFER TO INSTALLATION INSTRUCTIONS PRIOR TO ASSEMBLY.
  - DIALYSIS BOX CUTOUT IS PROVIDED. CLEARANCE AREA AROUND TO BE 17" x 14". CLIENT TO CONFIRM IF MORE CLEARANCE IS REQUIRED.
  - DIALYSIS BOX AND INSTALLATION PROVIDED BY OTHERS.
  - GFCI RECEPTACLES AVAILABLE BY REQUEST AT AN ADDITION CHARGE.
  - HORIZONTAL OVERHANGING IS NOT SHOWN ON THE DRAWING. CUSTOMER TO CONFIRM REQUIRED HEIGHT BETWEEN THE CEILING AND TOP OF HEADWALL. MAX. 6" OVERHANG IS PROVIDED.
  - SCONCES TO BE PROVIDED AND INSTALLED BY OTHERS, BLOCKING AND PROVISION PROVIDED BY AMICO.

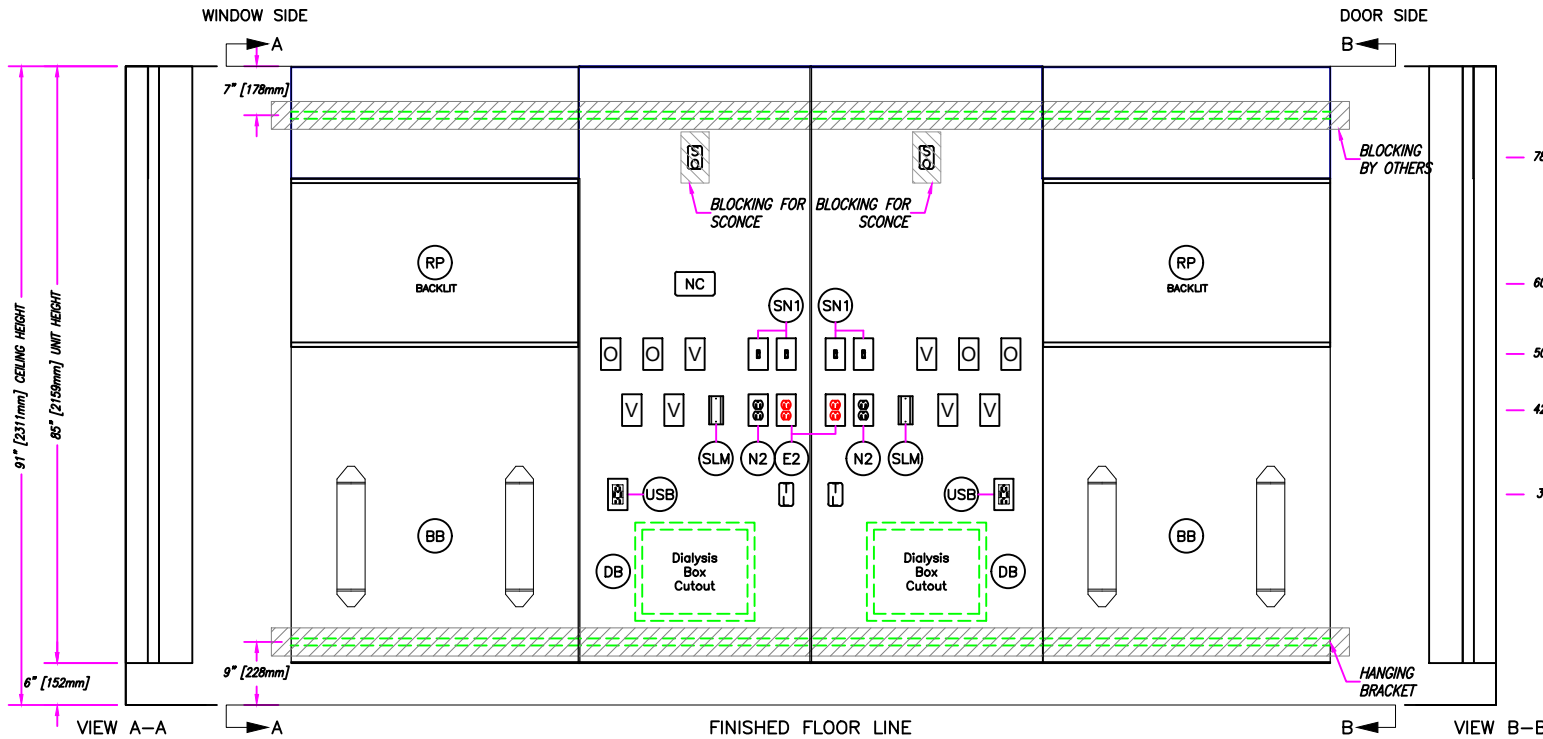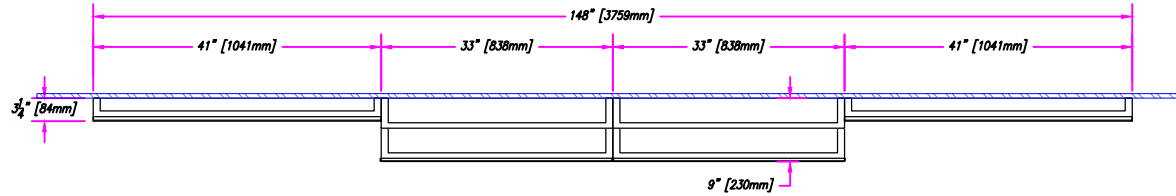

**IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.**

APPROVAL - PRINT AND SIGNATURE

DATE

PHONE NO.

HOSPITAL	RICHMOND UNIVERSITY MEDICAL CENTER	NURSE CALL	MFGR. : TBC	MODEL No. : TBC
LOCATION	STATEN ISLAND, NY	GAS OUTLETS	MFGR. : AMICO	TYPE CONNECTION : TBC
	UNIT AS SHOWN - N.T.S.	FINISH	TBC	CEILING HEIGHT 7' - 7"

85 Fulton Way  
Richmond Hill, Ontario  
L4B 2N4, CANADA  
Toll-Free: 1-877-482-6428(T)  
1-866-440-4986(F)  
Tel: (905) 764-0800  
Fax: (905) 764-0862

www.amico.com

QUOTE No.  
AC014104  
REV. BY: SLIU  
PROJECT PM: N/A  
DATE: Nov-23-2021  
REV. NO: 03